




SparMED Aps
Ryttermarken 2
3520 Farum
Denmark

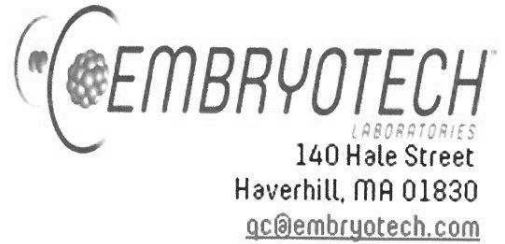

ELI Accession Number: SPAR-8639-0418

Date of completion: 04-20-2018

Lot number: 81403-MD

Reference number: OOMDW-120

Description of test article: Oosafe Disinfectant Wipes

Assay system requested by customer: An incubator was cleaned with test article. Post cleaning a culture plate was set up and one cell mouse embryos were cultured in the cleaned incubator for 96-hours.

Control assay method and results: 15 one cell (B6C3F1 X B6D2F1) embryos were cultured in triplicate micro drops of culture medium; control incubator ELI-182:

15 / 15 (100 %)

1-cell to 2-cell within 24 hr

15 / 15 (100 %)

1-cell to expanded blastocyst within 96 hr

For a valid assay, Embryotech™ requires at least 70% of one cell control embryos to develop to expanded blastocyst within 96-hours.

Test assay method and results: 21 one cell (B6C3F1 X B6D2F1) embryos were cultured in triplicate micro drops of culture medium while in incubator ELI-243 which was cleaned with the test article:

21 / 21 (100 %)

1-cell to 2-cell within 24 hr

21 / 21 (100 %)

1-cell to expanded blastocyst within 96 hr

Summary of observations: All test and control embryos were selected randomly from a common pool of freshly collected embryos. 100 percent of the control embryos developed to the expanded blastocyst stage within 96-hours. 100 percent of the embryos cultured in culture medium in the incubator that had been cleaned with the test article developed to the expanded blastocyst stage within 96-hours.

Signature
Study Director

04-20-2018

Date

Signature
Quality Reviewer

04-20-2018

Date